



Note: Refer to the C500 Owner's Manual page 12 for additional connection information.



McIntosh Laboratory, Inc. 2 Chambers Street Binghamton, New York 13903-2699 Phone: 607-723-3512 FAX: 607-724-0549 Part No. 04106800

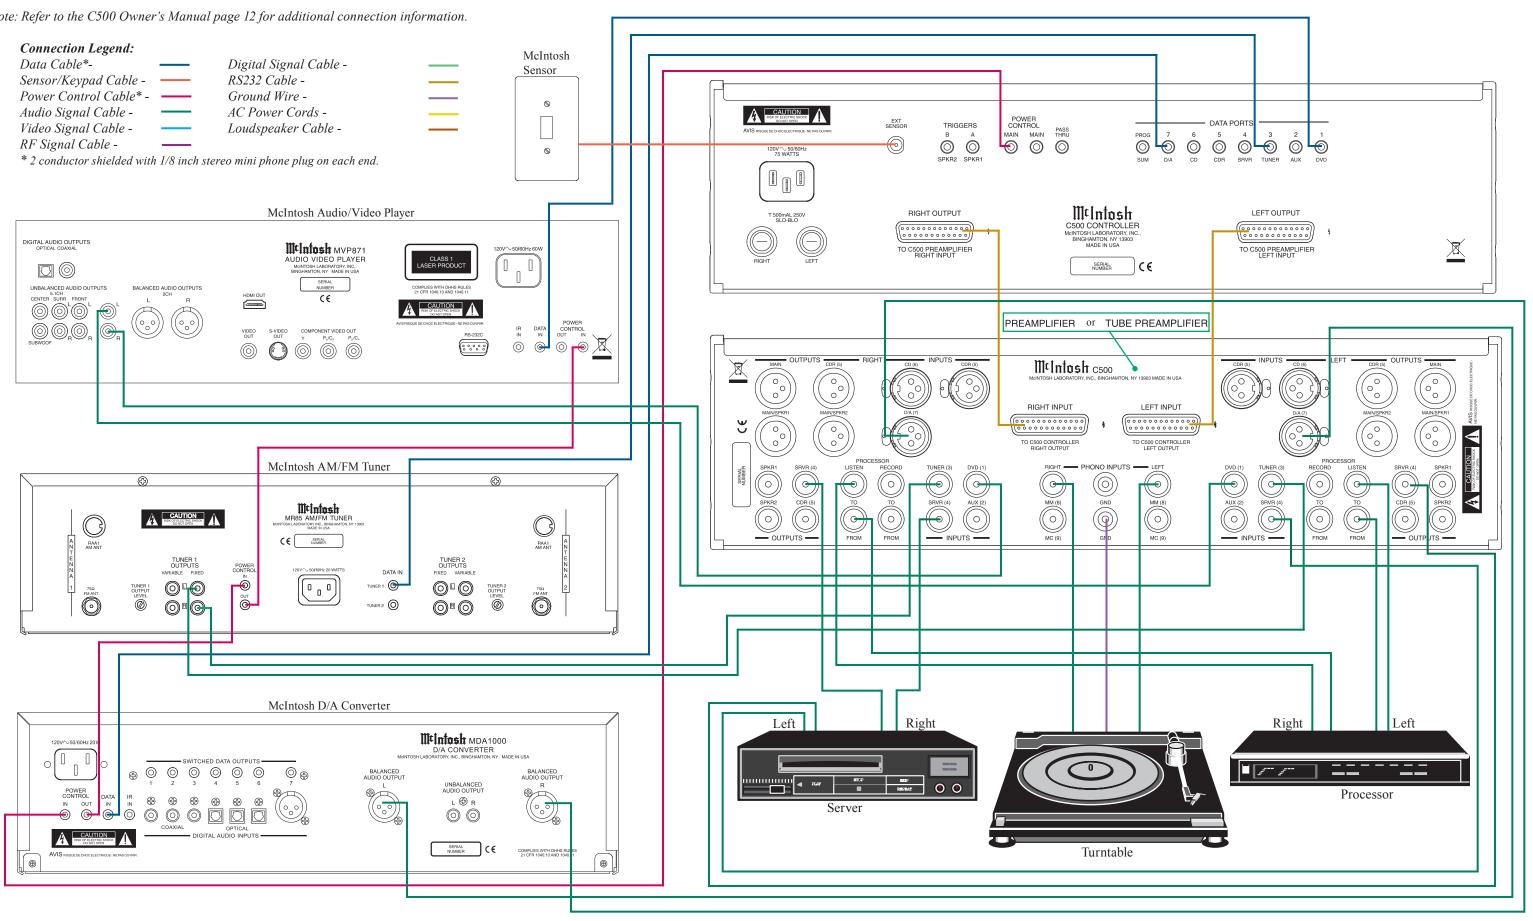

Note: Refer to the C500 Owner's Manual page 12 for additional connection information.



* 2 conductor shielded with 1/8 inch stereo mini phone plug on each end.

